Part Number: 186269506	Description: 2695 Separations Module
Tested By: SAIFUDDIN	Test Template Revision: 1.8
Serial Number: F18SM4699A	Test Station: Final-test-1
UUT Firmware: 3.04	System: 2695_1

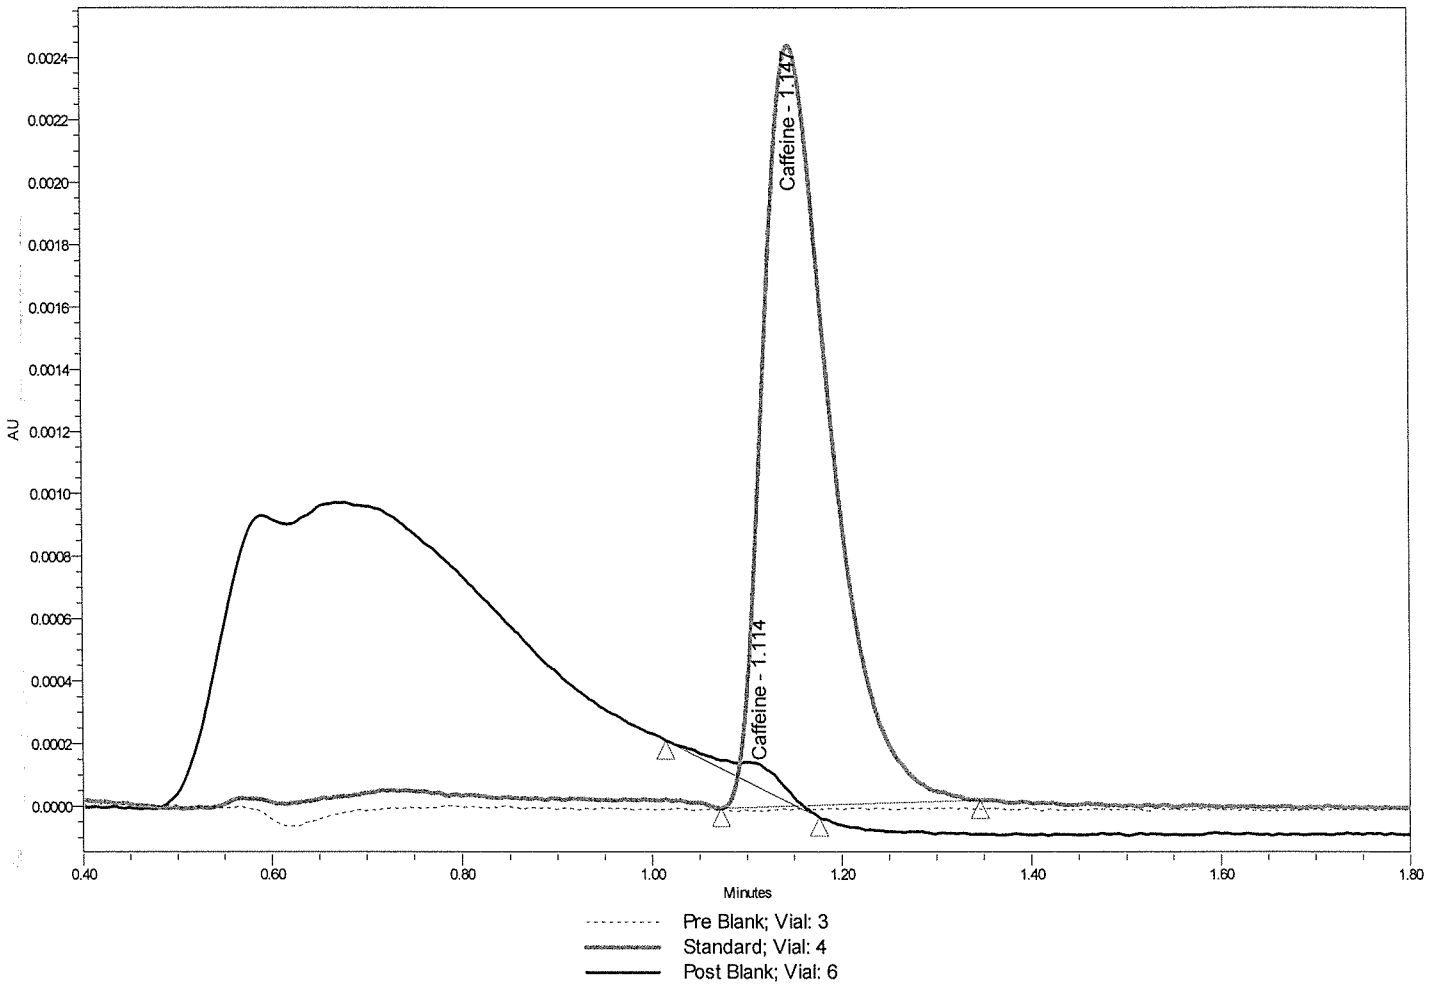

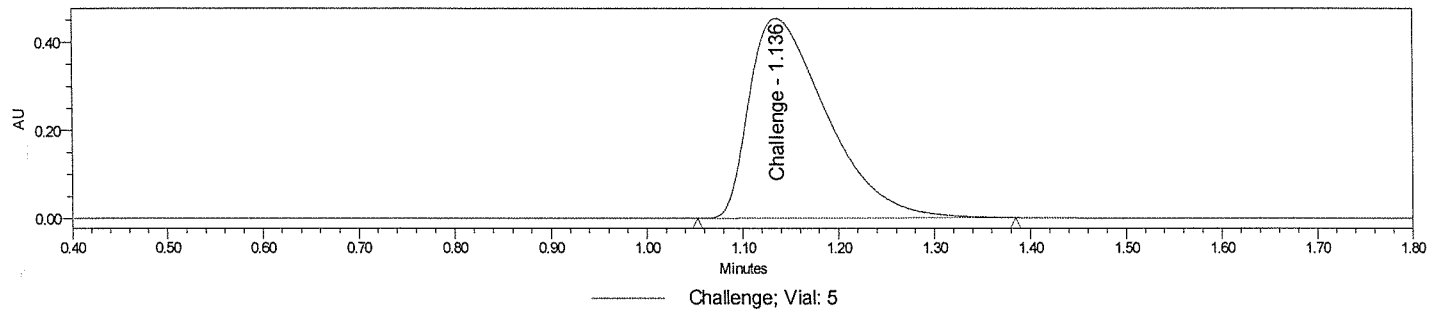

	Date Acquired	SampleName	Area	Percent
1	6/12/2018 7:31:28 PM SGT	Pre Blank		
2	6/12/2018 7:34:09 PM SGT	Standard	11992	0.0100
3	6/12/2018 7:36:53 PM SGT	Challenge	2554467	
4	6/12/2018 7:52:50 PM SGT	Post Blank	303	0.0003

Carryover Test:
PreBlank injection (to establish system cleanliness)
Standard (0.4 PPM) Caffeine injection
Challenge injection (10,000 X Standard = 4,000 PPM)
PostBlank injection
Carryover (%) = Carryover Area/Standard Area * 0.010

Specification: Post Blank Percent < 0.002
(or Blank peak(s) missing/blank)

This Test Record and any data contained within it are proprietary to Waters Corporation and must be retained by Waters for the time period prescibed in its Quality Records Retention Policy. If any of the individual tests fail; a note must be referenced that details the work performed to correct that specific deficiency. An overall failure indicates a special circumstance in which case a complete retest is to be done. A second form is required to document that testing; the initial form must be attached and retained.