
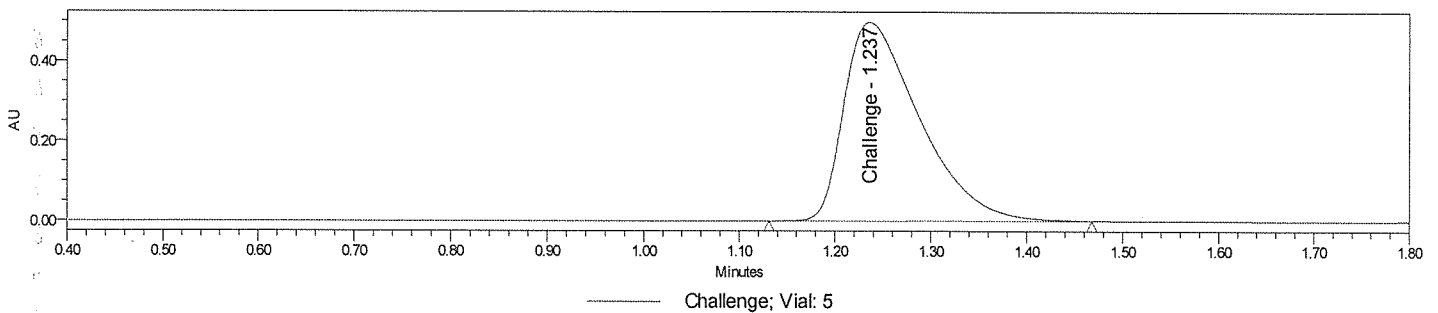


Part Number: 186269505
 Tested By: CHONG WOUI KHIP
 Serial Number: F18SM7140A
 UUT Firmware: 3.04

Description: 2695 Separations Module
 Test Template Revision: 1.8
 Test Station: Final-test-3
 System: 2695_4

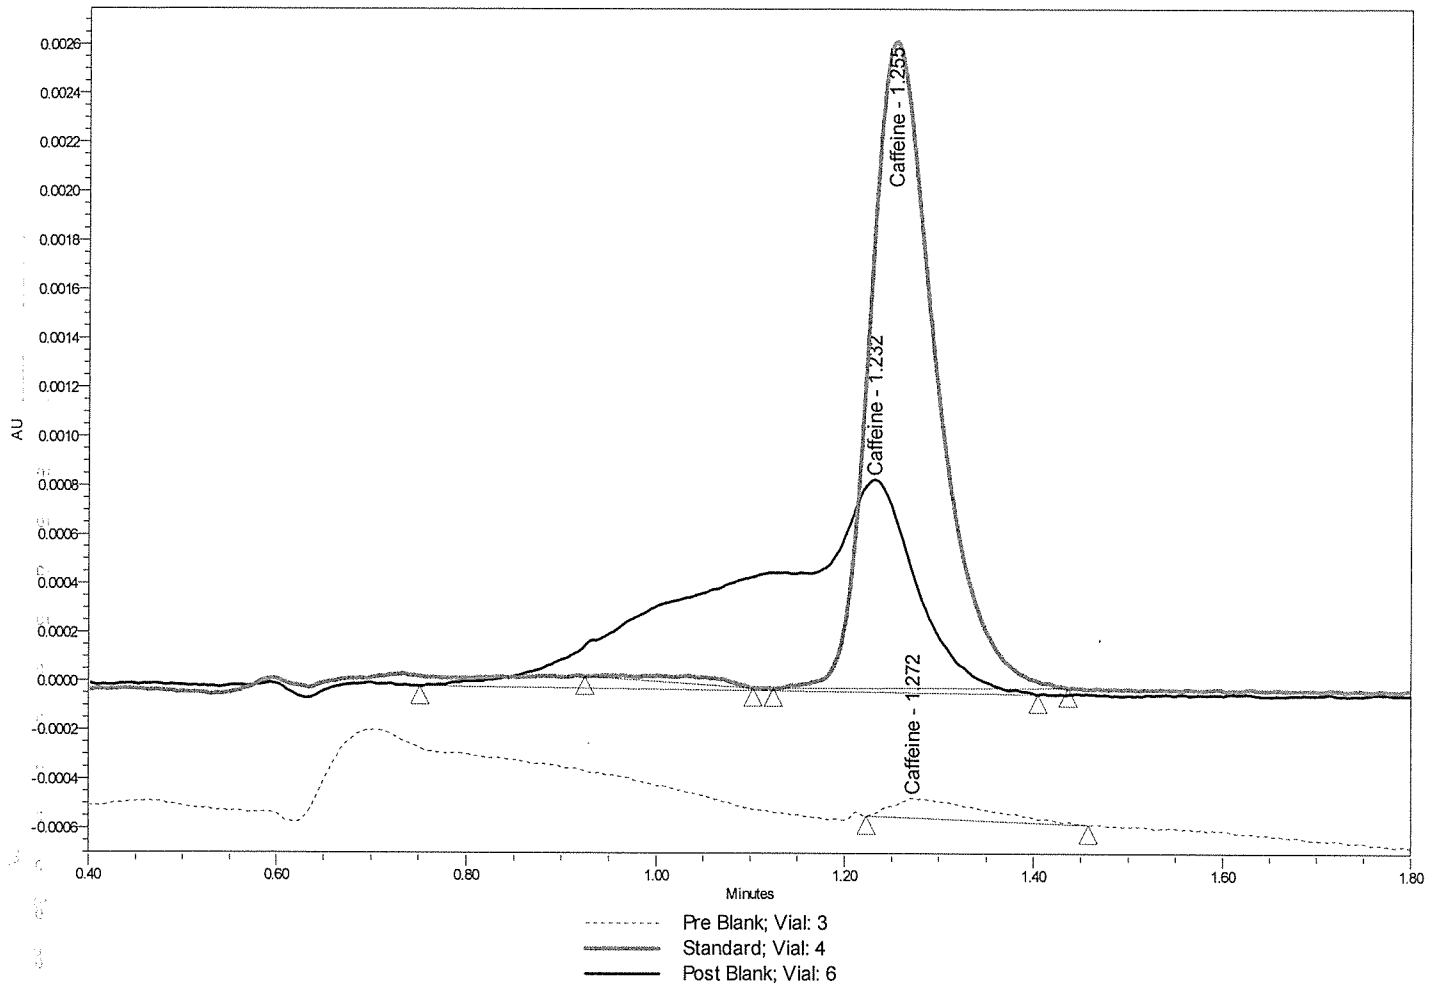

	Date Acquired	SampleName	Area	Percent
1	6/18/2018 2:56:46 PM SGT	Pre Blank	551	0.0004
2	6/18/2018 2:59:28 PM SGT	Standard	12877	0.0100
3	6/18/2018 3:02:10 PM SGT	Challenge	2725509	
4	6/18/2018 3:18:05 PM SGT	Post Blank	11318	0.0088



Carryover Test:
 PreBlank injection (to establish system cleanliness)
 Standard (0.4 PPM) Caffeine injection
 Challenge injection (10,000 X Standard = 4,000 PPM)
 PostBlank injection
 $\text{Carryover (\%)} = \frac{\text{Carryover Area}}{\text{Standard Area}} \times 0.010$

Specification: Post Blank Percent < 0.002
 (or Blank peak(s) missing/blank)

This Test Record and any data contained within it are proprietary to Waters Corporation and must be retained by Waters for the time period prescribed in its Quality Records Retention Policy. If any of the individual tests fail, a note must be referenced that details the work performed to correct that specific deficiency. An overall failure indicates a special circumstance in which case a complete retest is to be done. A second form is required to document that testing; the initial form must be attached and retained.

Part Number: 186269505
 Tested By: CHONG WOOL KHIP
 Serial Number: F18SM7140A
 UUT Firmware: 3.04

Description: 2695 Separations Module
 Test Template Revision: 1.8
 Test Station: Final-test-3
 System: 2695_4

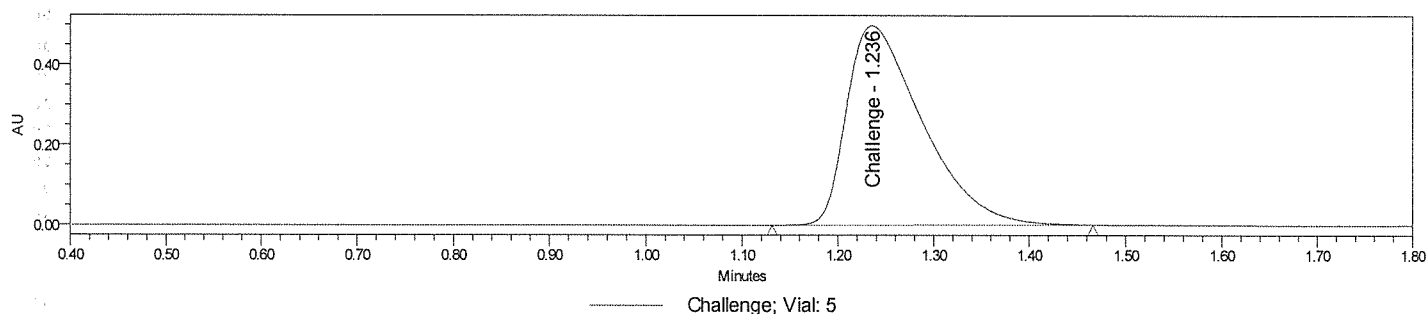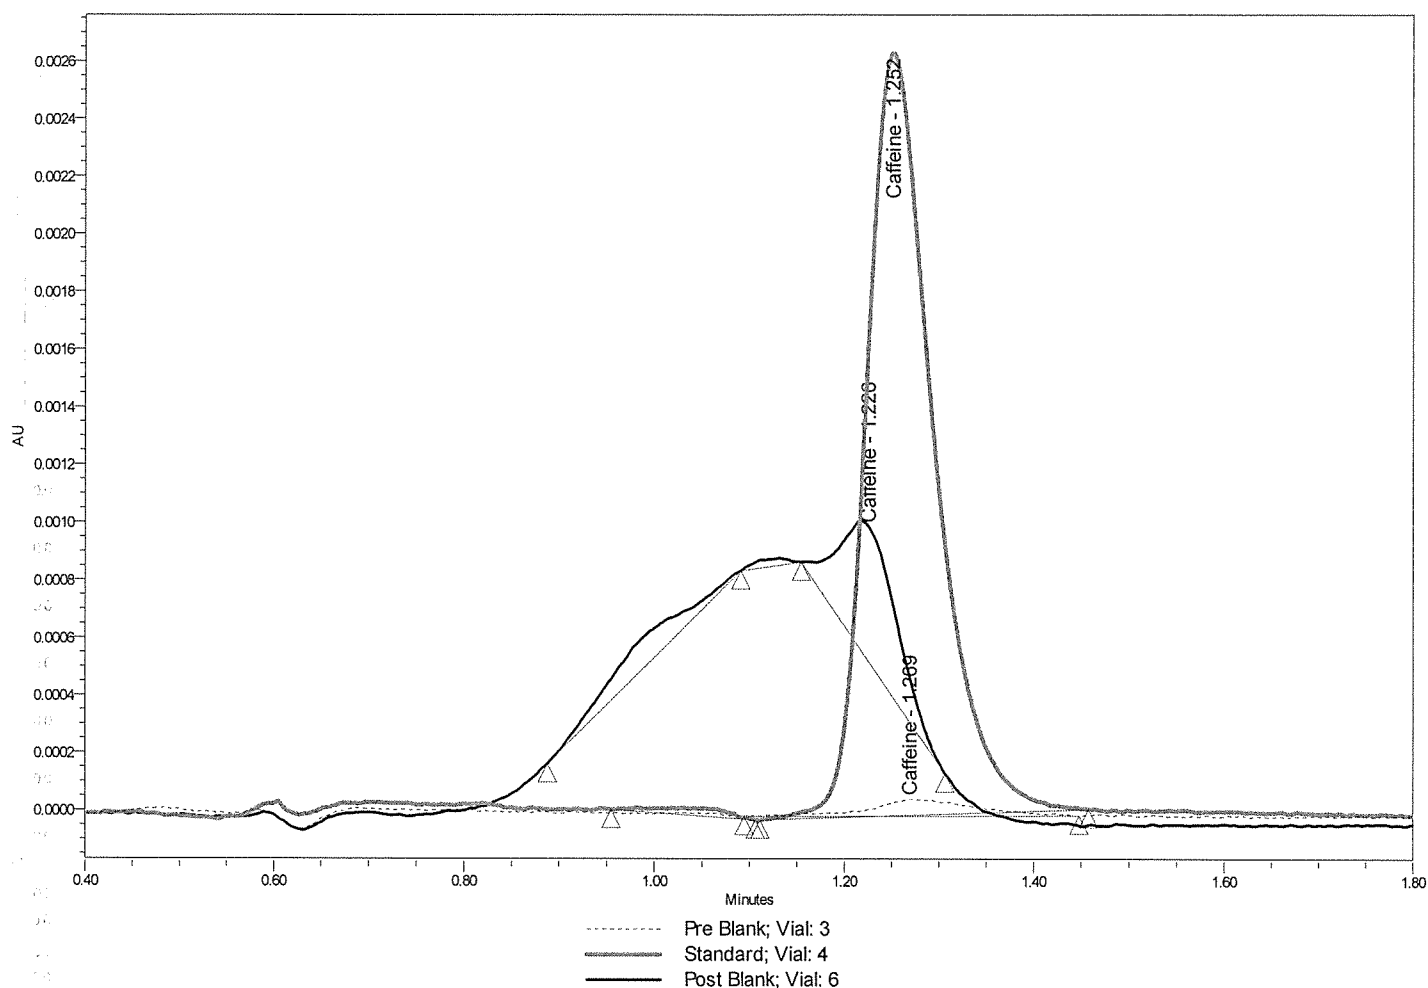

	Date Acquired	SampleName	Area	Percent
1	6/18/2018 2:27:31 PM SGT	Pre Blank	466	0.0004
2	6/18/2018 2:30:13 PM SGT	Standard	13038	0.0100
3	6/18/2018 2:32:56 PM SGT	Challenge	2732325	
4	6/18/2018 2:48:52 PM SGT	Post Blank	1971	0.0015

Carryover Test:
 PreBlank injection (to establish system cleanliness)
 Standard (0.4 PPM) Caffeine injection
 Challenge injection (10,000 X Standard = 4,000 PPM)
 PostBlank injection
 $\text{Carryover (\%)} = \frac{\text{Carryover Area}}{\text{Standard Area}} \times 0.010$

Specification: Post Blank Percent < 0.002
 (or Blank peak(s) missing/blank)

This Test Record and any data contained within it are proprietary to Waters Corporation and must be retained by Waters for the time period prescribed in its Quality Records Retention Policy. If any of the individual tests fail, a note must be referenced that details the work performed to correct that specific deficiency. An overall failure indicates a special circumstance in which case a complete retest is to be done. A second form is required to document that testing; the initial form must be attached and retained.