
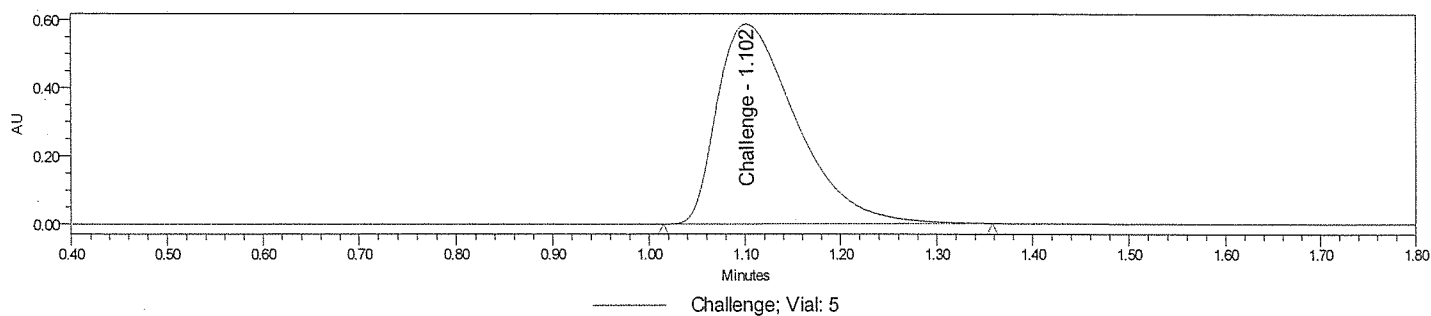


Part Number: 186269505
 Tested By: CHONG WOOL KHIP
 Serial Number: F18SM7119A
 UUT Firmware: 3.04

Description: 2695 Separations Module
 Test Template Revision: 1.8
 Test Station: Final-test-5
 System: 2695_1

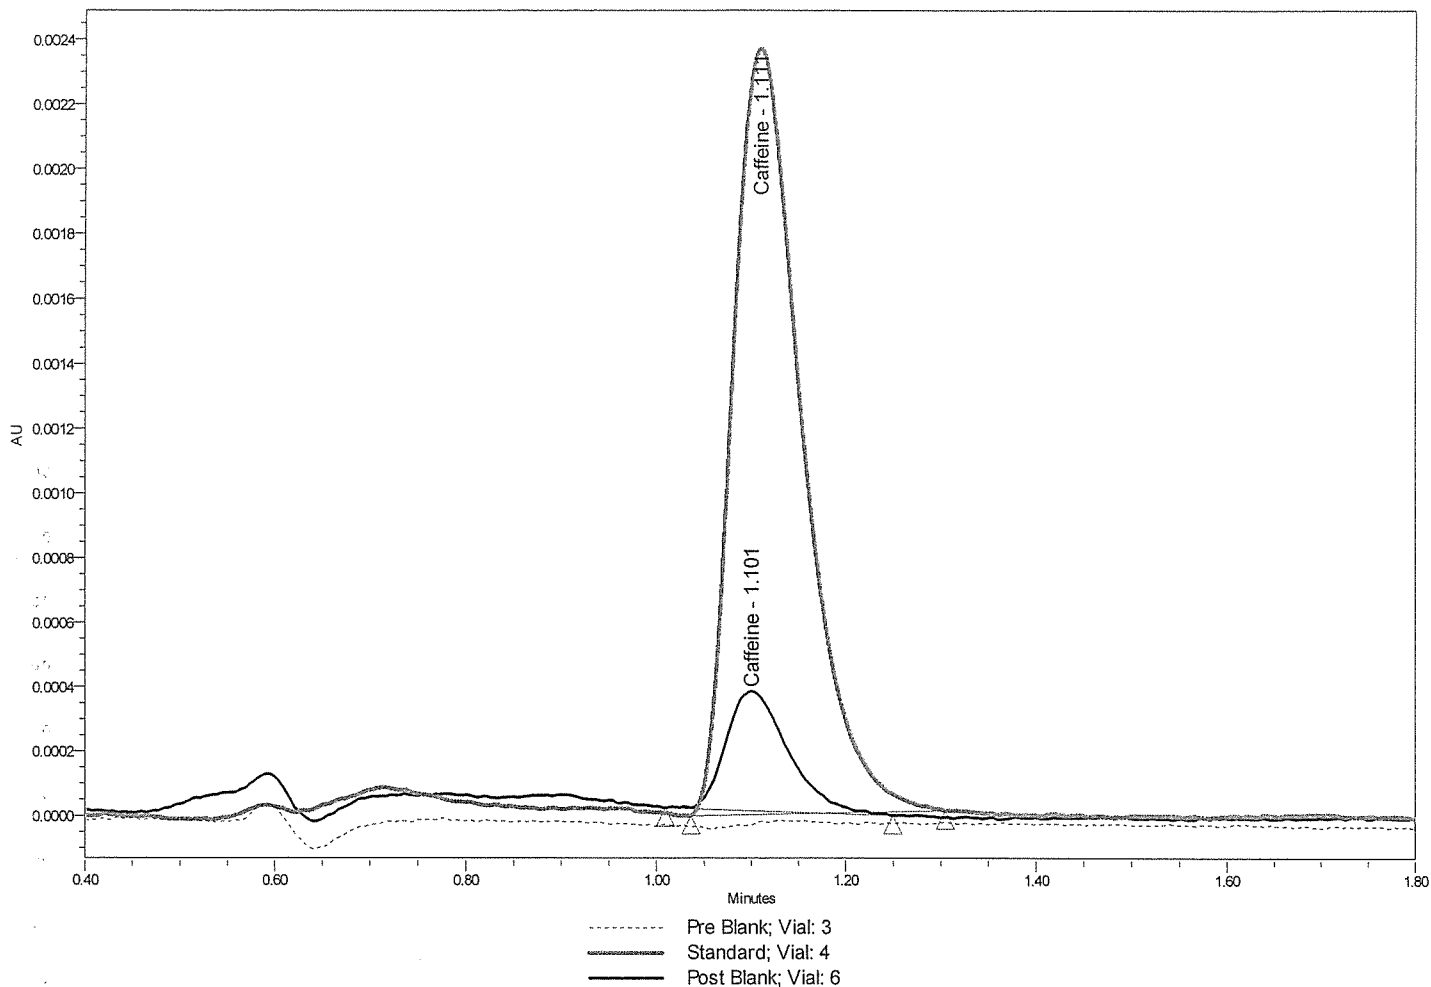

	Date Acquired	SampleName	Area	Percent
1	6/18/2018 11:18:43 PM SGT	Pre Blank		
2	6/18/2018 11:21:24 PM SGT	Standard	12075	0.0100
3	6/18/2018 11:24:06 PM SGT	Challenge	3376917	
4	6/18/2018 11:40:02 PM SGT	Post Blank	1692	0.0014



Carryover Test:
 PreBlank injection (to establish system cleanliness)
 Standard (0.4 PPM) Caffeine injection
 Challenge injection (10,000 X Standard = 4,000 PPM)
 PostBlank injection
 $\text{Carryover (\%)} = \frac{\text{Carryover Area}}{\text{Standard Area}} \times 0.010$

Specification: Post Blank Percent < 0.002
 (or Blank peak(s) missing/blank)

This Test Record and any data contained within it are proprietary to Waters Corporation and must be retained by Waters for the time period prescribed in its Quality Records Retention Policy. If any of the individual tests fail, a note must be referenced that details the work performed to correct that specific deficiency. An overall failure indicates a special circumstance in which case a complete retest is to be done. A second form is required to document that testing; the initial form must be attached and retained.

Part Number: 186269505
 Tested By: CHONG WOOL KHIP
 Serial Number: F18SM7119A
 UUT Firmware: 3.04

Description: 2695 Separations Module
 Test Template Revision: 1.8
 Test Station: Final-test-5
 System: 2695_1

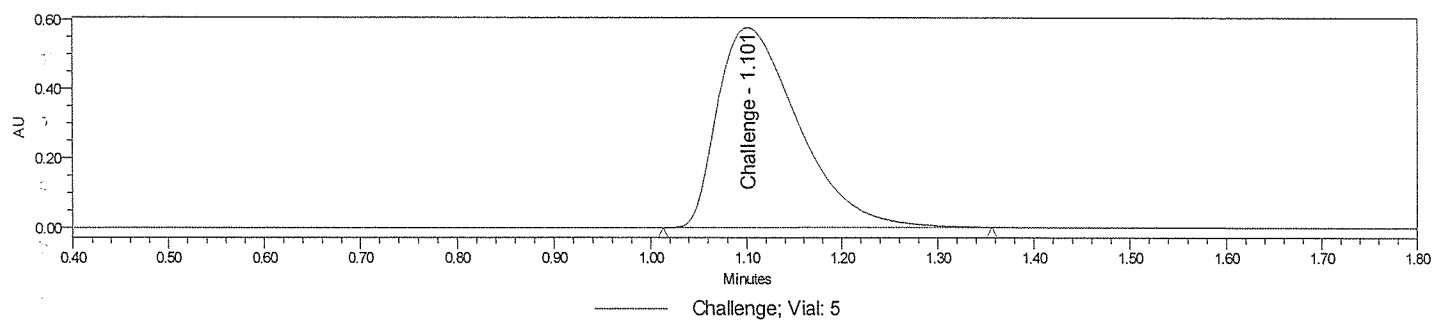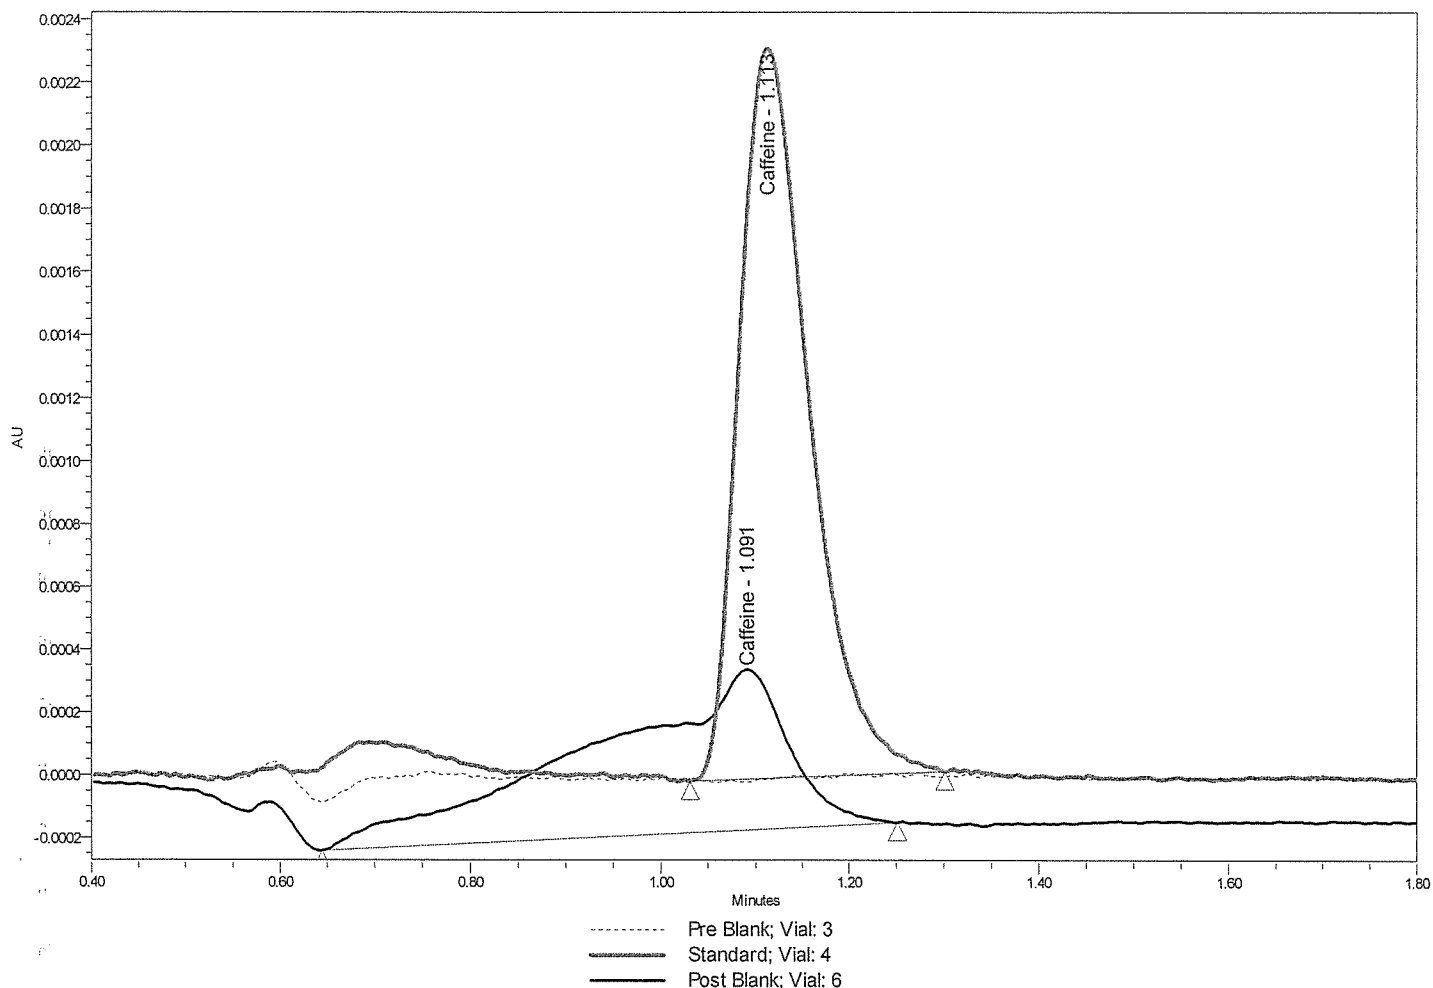

	Date Acquired	SampleName	Area	Percent
1	6/18/2018 6:35:18 PM SGT	Pre Blank		
2	6/18/2018 6:37:59 PM SGT	Standard	12068	0.0100
3	6/18/2018 6:40:43 PM SGT	Challenge	3374188	
4	6/18/2018 6:56:38 PM SGT	Post Blank	7532	0.0062

Carryover Test:
 PreBlank injection (to establish system cleanliness)
 Standard (0.4 PPM) Caffeine injection
 Challenge injection (10,000 X Standard = 4,000 PPM)
 PostBlank injection
 Carryover (%) = Carryover Area/Standard Area * 0.010

Specification: Post Blank Percent < 0.002
 (or Blank peak(s) missing/blank)

This Test Record and any data contained within it are proprietary to Waters Corporation and must be retained by Waters for the time period prescribed in its Quality Records Retention Policy. If any of the individual tests fail; a note must be referenced that details the work performed to correct that specific deficiency. An overall failure indicates a special circumstance in which case a complete retest is to be done. A second form is required to document that testing; the initial form must be attached and retained.