



Acquity Column Manager Test Record

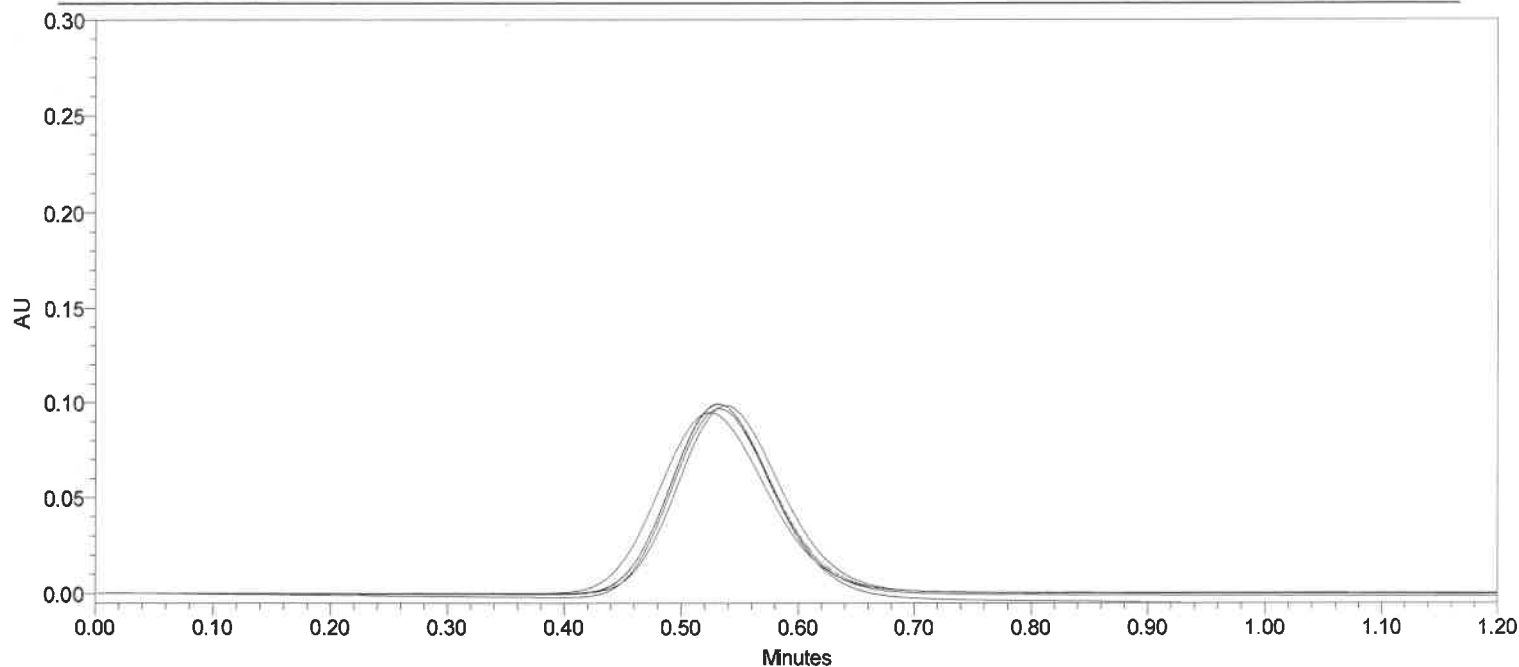


Peak Data

	Date Acquired	Sample Name	Retention Time (min)	Area (μV*sec)	Width @ 4.4%	Asym @ (4.4)^2	USP Tailing
1	4/15/2021 11:12:29 AM SGT	Column 1	0.533	625441	0.218	1.928	1.186
2	4/15/2021 11:16:08 AM SGT	Column 2	0.532	624554	0.214	1.780	1.161
3	4/15/2021 11:19:48 AM SGT	Column 3	0.538	622980	0.217	1.774	1.160
4	4/15/2021 11:23:25 AM SGT	Column 4	0.532	620378	0.215	1.778	1.161
5	4/15/2021 11:27:07 AM SGT	Column BP	0.525	622566	0.225	1.710	1.149
Max						1.928	1.186

Pressure @ 50 ul/min

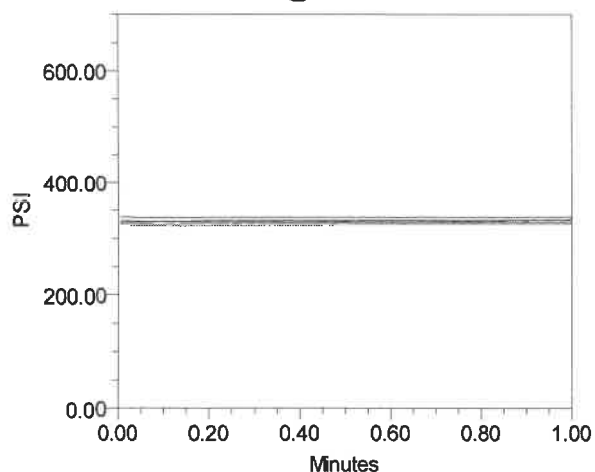

Pressure @ 0.5 ml/min

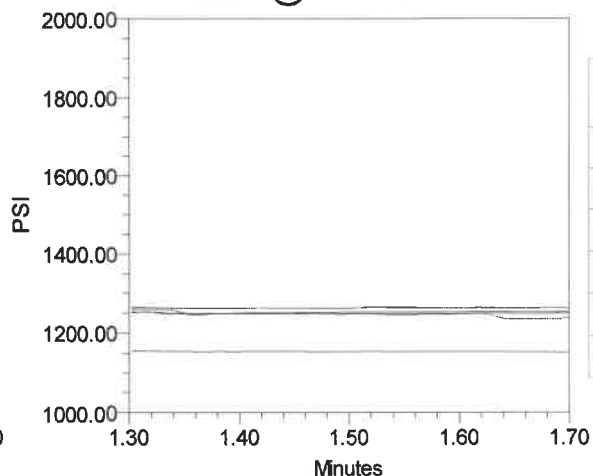

Pressure @ 0.5 ml/min

	Sample Name	Pressure (PSI)
1	Column 1	1326
2	Column 2	1368
3	Column 3	1264
4	Column 4	1283
5	Column BP	1164
Max		1368

Sample Set: C21UPM036G

Specifications: Asym @ 4.4^2 < 2.75, USP Tailing < 1.35